

## SARS-CoV-2 Antigen

**NOT FOR AT-HOME TESTING!  
FOR PROFESSIONAL USE ONLY!**

# SARS-CoV-2 Ag Rapid Test

VivaDiag™ SARS-CoV-2 Ag Rapid Test is for the rapid, qualitative detection of the nucleocapsid protein antigen from SARS-CoV-2 in human nasal swab, oropharyngeal swab or nasopharyngeal swab specimen. The test is for *in vitro* diagnostic use only.


## Specification

Test Principle	Colloidal gold
Sample Type	Nasal swab, oropharyngeal swab or nasopharyngeal swab
Sample Volume	60 µL
Test Time	15 min
Operation Temperature	15-30°C
Storage Temperature	2-30°C
Shelf Life (Unopened)	24 months




## Steps for a Single Test

### Specimen Collection

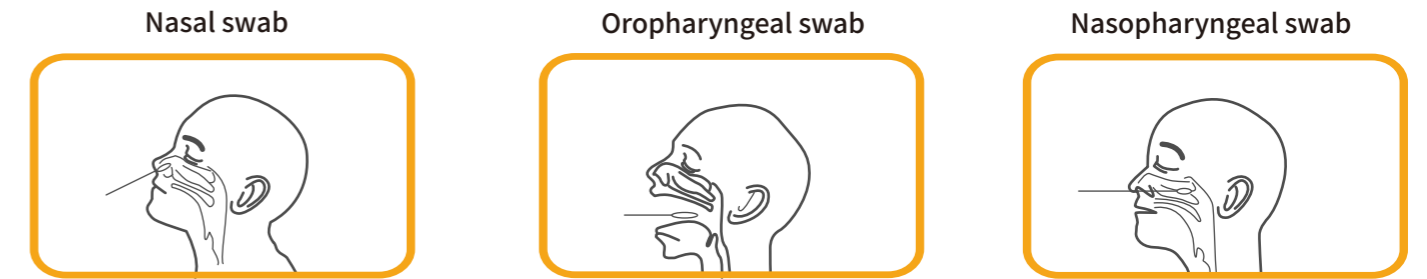


### Solution Preparation

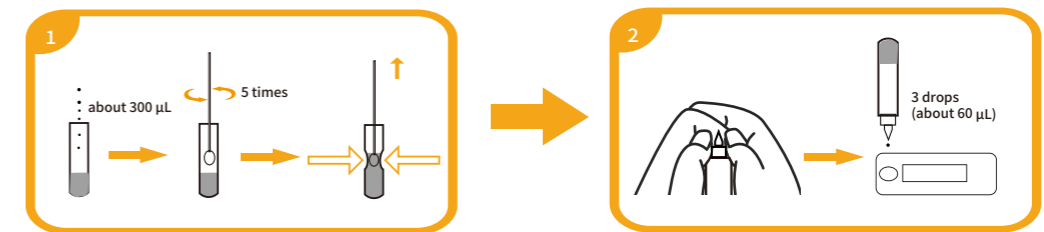

1. Prepare the specimen


2. Apply the extracted specimen

### Detection

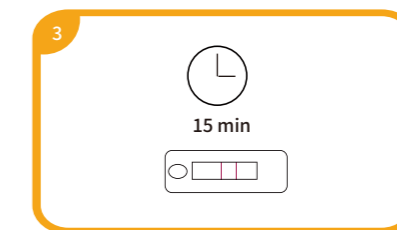


3. Read the test result


### Result Interpretation



Positive



Negative



Invalid

Note: The VivaDiag™ SARS-CoV-2 Ag Rapid Test has ONLY been designed to act as a supplementary test for suspected cases of negative coronavirus nucleic acid detection or in conjunction with nucleic acid detection in the diagnosis of suspected cases. Results from nucleocapsid protein antigen testing should not be used as the sole basis to diagnose or exclude SARS-CoV-2 (COVID-19) infection or to inform infection status.